

A THERMAL FLOWMETER FOR ESTIMATING THE RATE OF XYLEM SAP ASCENT IN TREES

Robert H. Swanson

THIS FILE COPY MUST BE RETURNED

TO: INFORMATION SECTION,
NORTHERN FOREST RESEARCH CENTRE,
5320-122 STREET,
EDMONTON, ALBERTA,
T6H 3S5

REPRINTED
FROM

FLOW

ITS MEASUREMENT AND CONTROL IN SCIENCE AND INDUSTRY
VOL. 1

Rodger B. Dowdell
Editor-in-Chief

Sponsored by: American Society of Mechanical Engineers, National Bureau of Standards,
American Institute of Physics, Instrument Society of America



INSTRUMENT
SOCIETY
OF AMERICA

A THERMAL FLOWMETER FOR ESTIMATING THE RATE OF XYLEM SAP ASCENT IN TREES

ROBERT H. SWANSON

*Canadian Forestry Service
Edmonton, Alberta, Canada*

Distortion in heat diffusion patterns in thermally homogenous media can be used to indicate the influence of external stimuli. Considering a living tree stem as such a medium thermal diffusion patterns following an injected heat pulse are related to water evaporated from the leaf surfaces which results in the vertical movement of water in the stem. The equation $v = [(4\pi kt)^{-1} Q] \exp - [(x - HPVt)^2 (4kt)^{-1}]$ describes the temperature (v) at any point (x) in a medium moving at velocity (V), initially at thermal equilibrium and of diffusivity (k) for any time greater than $t = 0$. The simultaneous solution of two such equations for points x, x' ($x \neq x'$), results in an equation for heat pulse velocity (HPV): $HPV = (x - x') (2t_0)^{-1}$, where t_0 is the time for $v = v'$ following the instantaneous release of a quantity of heat (Q) at $x = 0$. Heat pulse velocity is a quantitative indicator of the rate of upward water movement. Instrumentation to measure heat pulse velocity consists of a heat source, temperature detector, and a timer. Practical circuits, schematics, and drawings for a portable field instrument are given.

INTRODUCTION

Distortion in heat diffusion patterns in thermally homogenous media can be used to indicate the influence of external stimuli. Measuring water flow through porous media is one application. A porous medium of interest to forest hydrologists is a tree stem. Water moves upward from the roots via the stem in response to evaporation at the leaf surfaces. The amount of water evaporated and the response of evaporation rate to various climatic parameters are useful information for managing forests as watersheds. One means of obtaining such information is with a thermal flowmeter.

INSTRUMENTATION

A thermal flowmeter consists of two devices—(1) a means of injecting or creating heat within a flowing medium, and (2) some means of registering its rate of diffusion or tracing it downstream. A flowmeter for a tree stem is shown in Fig. 1. Basically, it consists of a heater (H) with temperature measuring probes at (x) and (x').

In a pure convective medium, velocity between points x, x' would be simply the distance $x - x'$ divided by the time from heat creation at H to its onset at x . A tree is not a purely convective medium. In fact, a greater proportion of heat will reach both points x and x' by conduction

than by convection. The theoretical derivation of the formula to describe how heat both convects and conducts in this medium are covered elsewhere.¹ With the probe configuration of Fig. 1, heat pulse velocity (HPV), a parameter closely related to mass flow, can be gotten with simple temperature difference measurements at points x and x' and the time for equal temperature at these two points after an initial difference because of a heat pulse created at H.

The temperature (v) for any time, $t \neq 0$, at point x downstream, is described by Eq. (1):

$$v = \frac{Q}{4\pi kt} \exp - \left[\frac{(x - HPVt)^2 + y^2}{4kt} \right] \text{ } ^\circ\text{C} \quad (1)$$

A second equation can likewise be written for an upstream point x' . Simultaneous solution for HPV at the time to when $v = v'$ ($t \neq 0, x \neq x'$) yields Eq. (2), x, x' in cm, t in seconds.

$$HPV = (x - x')/2t_0 \text{ cm/s} \quad (2)$$

or

$$HPV = 1800 (x - x')/t_0 \text{ cm/h} \quad (3)$$

(the "y" component is assumed zero by making all measurements in the $y = 0$ plane).

Instrumentation to utilize Eq. (2) to estimate heat pulse velocities is straightforward and

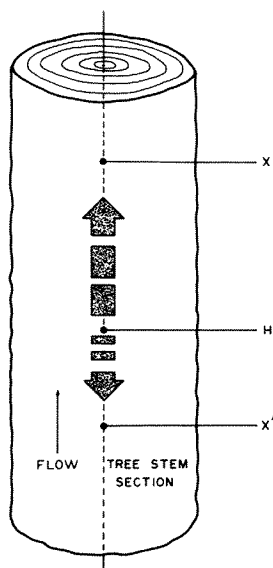
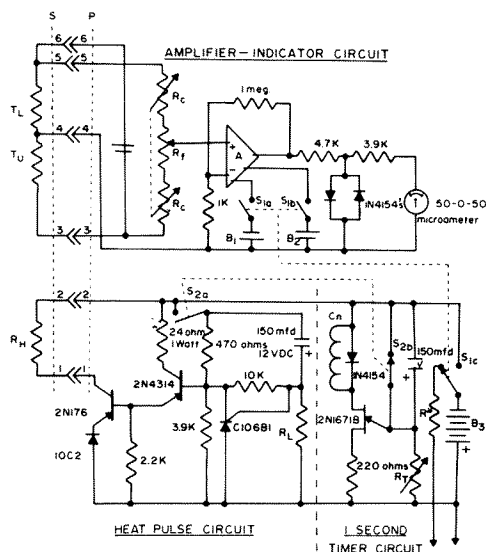


Fig. 1. Thermal flowmeter for a tree stem.

simple. Probes can be any temperature sensing and display device capable of detecting and indicating temperature differentials of 0.001°C . Thermistors have been used with the greatest success, but thermocouples are also suited if precautions are taken to eliminate thermal exchanges outside of the metered section. A second timer and a battery to create a momentary heat pulse are the only other requirements. A schematic diagram of the most recent complete instrument package in use by the author is shown in Fig. 2. Figure 3 shows heat source construction. Figure 4 shows thermistor probe construction. These probes are best left permanently in place in a tree stem. A socket mounted at each metering point allows more than one set of probes to be serviced by a single indicating-timing package.

FLOW ESTIMATES

The continuity equation $Q = AV$ requires a knowledge of the average velocity V through some cross section area A in order to calculate quantity Q . In a tree stem, the same is true. Heat pulse velocity is measured using the instrumentation of Figs. 2, 3, and 4. However, in order to obtain average HPV and A , we must assume some properties of the flow system. The following would apply to Lodgepole pine or Engelmann spruce tree of 10-cm diameter or larger.



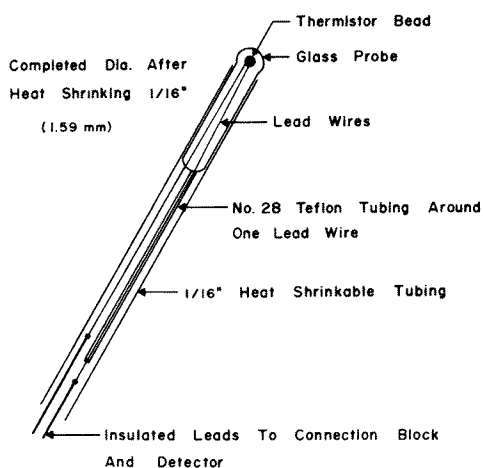


Fig. 4. Thermistor probe construction.

First we assume that the velocity distribution across the water conducting cross section is parabolic.² To describe average heat pulse velocity over a radial cross section two concurrent HPV measurements, at 1.0 and 2.0 cm deep are made. A second set of measurements on the opposite side of the tree should also be made to allow for departure from circular symmetry in the stem. For each set of measurements, compute the average velocity and its physical position in the cross section. To do so it will be necessary to derive the equation for a parabola through the two measured points (1.0, HPV₁), (2.0 HPV₂) and the origin where the HPV is assumed zero (0,0). The equation for the shape factor (*a*), peak heat pulse velocity (PHPV), and depth at which the peak occurred (Dp) are

$$a = -0.50 / (2\text{HPV}_1 - \text{HPV}_2) \quad (4)$$

$$\text{Dp} = 1 - a\text{HPV}_2 \text{ cm} \quad (5)$$

$$\text{PHPV} = \text{Dp}^2 / (-4a) \text{ cm/h} \quad (6)$$

Average heat pulse velocity ($\overline{\text{HPV}}$) is defined by (7).

$$\overline{\text{HPV}} = (2 \text{ PHPV}) / 3 \quad (7)$$

The conducting cross-sectional area (CA) of the tree is computed from the overall stem diameter measurement (inside bark) and the average Dp obtained from the two measurements above.

$$\text{CA} = 2\pi\text{Dp}(D - 2\text{Dp}) \quad (8)$$

As an example, using actual field data for HPV and diameter: $D = 22.8$ cm, side 1: HPV_{1,2} = 6.0, 6.0; side 2: HPV_{1,2} = 6.7, 6.4.

Side 1: $a = -0.083$, Dp = 1.50 cm, PHPV = 6.8 cm/h.

Side 2: $a = -0.0714$, Dp = 1.46 cm, PHPV = 7.4 cm/h.

$$\overline{\text{HPV}} = (6.8 + 7.4) / 3 = 4.7 \text{ cm/h}$$

$$\text{CA} = (6.28) (1.48) (22.8 - 2.96) = 184 \text{ cm}^2$$

therefore Q, total flow would be: $(4.7) (184) = 864.8 \text{ cc/h}$.

DISCUSSION

Relative estimates are computable directly as above. The question with this or any flowmeter is how accurate are the estimated compared to actual flow? In the above estimates, there are three potential error sources: HPV may not be a valid indicator of flow/unit area cross section; HPV estimates may not be true magnitude due to the effect of the probes on the living flow system; the assumed parabolic heat pulse velocity-depth relationship may not be true, causing errors in both average heat pulse velocity and area.

Heat Pulse Velocity as an Indicator of Flow per Unit Cross Section

According to Marshall,¹ heat pulse velocity is a weighted average of the nonmoving wood and moving sap acting together as a single medium. It is defined by Eq. (8).

$$\text{HPV} = a u \text{PsCs} / \text{Pc} \text{ cm/s} \quad (9)$$

where:

a = the fraction of any plane area perpendicular to the x axis occupied by sap streams

u = actual sap speed cm/s

PsCs = density and specific heat of sap

Pc = density and specific heat of combined sap and wood.

The interpretation of HPV as a velocity stems from the interpretation of "*a*" as a unitless fraction. That is, *a* = sq. cm of sap stream

divided by sq. cm of wood, i.e., sq. cm/sq. cm = 1. Thus, HPV derives its units solely from sap velocity "u".

On the other hand, HPV can be interpreted in the same manner as a flux per unit area by simply failing to cancel the units (sq. cm) (cm/s) (Sq. cm)⁻¹ = (cc) (s)⁻¹ (sq. cm)⁻¹.

The correct interpretation may never be resolved. There is evidence for both. Marshall¹ derived a second term, sap flux (SF) that he intended heat pulse velocities to be converted to before they were used to compare flow between or compute actual flow within tree stems.

$$SF = HPV (Mc + 0.33)P (cc) (s)^{-1} (cm)^{-2} \quad (10)$$

where Mc = moisture content expressed as a decimal fraction measured on a dry weight base, P = oven-dried weight of wood divided by green volume.

Both Mc and P vary with time. Thus, both "a" and "u" of Eq. (9) vary with time too. A comparison of actual and calculated flows using (HPV) × (A) and (SF) × (A) is shown in Fig. 5. The relationship is rectilinear using heat pulse velocity, curve linear using sap flux. During the study conducted to obtain the data for Fig. 5, the moisture content varied from 1.01 to 0.75, the density from 0.46 to 0.52. My conclusion from Fig. 5, is that heat pulse velocity measurements already vary in magnitude in accordance

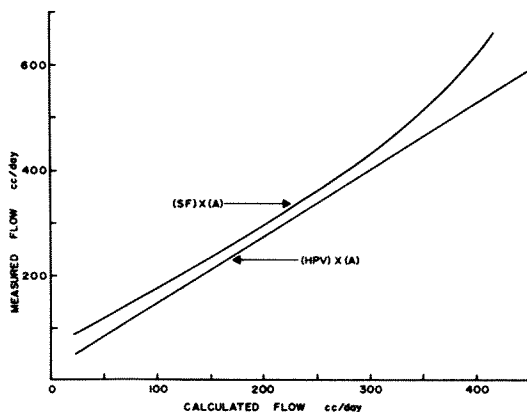


Fig. 5. Flow volume vs (sap flux) × (area) and (heat pulse velocity) × (area).

with changes in moisture content and density, and that conversion to sap flux introduces this variation a second time, creating the curve linearity.

More important than the curve linearity, is the lack of 1:1 correspondence between either (HPV) × (A) or (SF) × (A). Both underestimate the actual amount of water flowing through the measurement cross section. Heat pulse velocity × area underestimates actual flow by 75 percent; sap flux × area by 65 percent. A reason for these underestimates is discussed below.

Effect of Probes' Size on Measured Magnitude

Upward flow in a living tree stem is in response to evaporation at the leaf surfaces. The water is pulled upward in coniferous trees via a series of conducting cellular structures called tracheids. In pine, tracheids are 4 to 6 cm long. Water flows from tracheid to tracheid both vertically and to a much lesser extent, horizontally, through bordered pits at the tapered junctions. Each bordered pit is equipped with a valve-like structure that remains open as long as the pressure on both sides of it remains relatively equal. Any disruption of flow through a tracheid or group of tracheids results in closing of the disturbed flow path.

Both thermistor and heat probes must be inserted among the tracheids to meter the flow through them. While it might be possible to sharpen the probes to such an extent that they could be inserted without severing any tracheids, the usual procedure is to drill holes and insert fairly blunt probes to the desired length. Drilling does disturb a considerable number of tracheids. This results in a drying of the water conducting elements immediately above and below the measurement plane. Figure 6 shows how such drying appears in dye staining patterns on instrumented cross sections. The dye pattern separated 2 to 3 cm below the lowest probe and stayed separated for about 3 cm above the highest probe. The width of the dried area is slightly greater than the diameter of the largest probe. In Fig. 6, all probes are 1 mm diameter, the dry area about 2 mm wide.

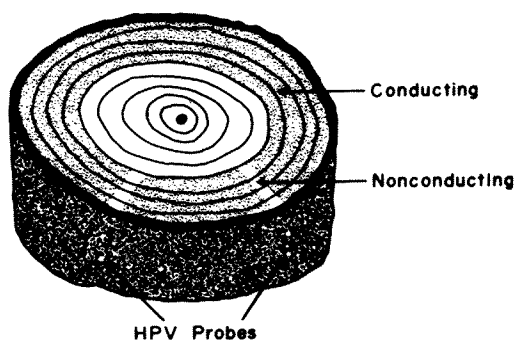


Fig. 6. Dye staining pattern within a cross section instrumented with heat pulse velocity measuring probes.

Figure 7 shows the area of wood about the probes that receives influence from the heat pulse. The most influenced area is immediately adjacent to the vertical plane of the heat source. Relative influence decreases rapidly both directions perpendicular to the heat source plane.

The response curve of Fig. 8 is not symmetrical. This is because the thermistor probes used to obtain these data were mounted in hypodermic needles and were influenced more by heat travelling along the butt toward the tip than by heat travelling through wood to the tip. Less conductive probes result in better symmetry. Regardless of symmetry, if we accept 5 percent relative response as being the minimum detectable with the indicating instrumentation, then the "sensed" area is roughly a rectangle, extending 0.75 cm in each side of the heat source.

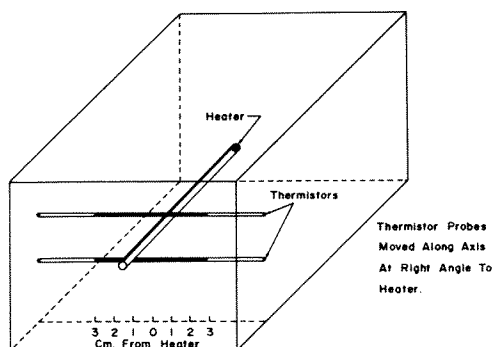


Fig. 7. Area in the y - z plane influenced by a heat source on the x axis. Diagrammatic sketch of measurement scheme.

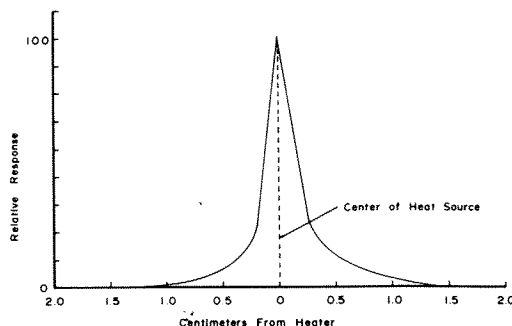


Fig. 8. Area in the y - z plane influenced by a heat source on the x axis. Graphical result.

Figure 6 shows that an area 2 mm wide, immediately adjacent to a probe set is not functioning in conducting water through the metered section. Comparing this information from that of Fig. 8 suggests that the most responsive portion of the sensitive area is not functioning. The area remaining after the 2 mm wide band is removed is 1.3 cm wide, or approximately 87 percent of the sensitive area is responsible for the heat pulse velocity measured. Assuming that the dried area is always twice the size of the largest probe helps explain the underestimate of Fig. 5. The thermistor probes for that study were 2.28 mm diameter: if an area 4.56 mm wide was not functioning, then only $1.044/1.500$ or 69 percent of the area was causing the heat pulse velocity readings. Thus, the 75 percent and 65 percent of actual flow, obtained by using $(HPV) \times (A)$ or $(SF) \times (A)$ are not out of line if a probe size correction based on twice the diameter is applied to those readings.

Other Potential Error Sources

A complete discussion of the evidence for assuming a parabolic heat pulse velocity-depth distribution is included elsewhere in these proceedings.² It will suffice to say here that this assumption is reasonable in light of the experimental evidence to date. More important are the sampling problems in obtaining heat pulse velocities at 1.0 and 2.0 cm deep. The interior of a tree is not homogeneous. As a tree grows, old knots, wounds, *et cetera*, are grown over and often not visible from the surface. The more limbs a tree species has, the greater the chance of encountering one of these imperfections. Their effect is similar to that of severing

several tracheids. Flow divides around the knot or wound area, leaving a nonconducting void immediately above and below.

In general, it is not possible to avoid such areas. Careful attention to probe placement to avoid visible defects is mandatory. However, a random sampling program and careful analysis of the collected data to detect obviously erroneous readings are the only way to insure representative data, free of bias.

What are "obviously erroneous readings"? Certainly, those which when analyzed using Eqs. (4), (5), and (6), produce a D_p much greater than one-fourth the total diameter of the tree. Only in very juvenile trees without developed heartwood would there be appreciable sap movement throughout the entire cross section. Also readings which produce an "a" greater than zero indicate an inverted velocity distribution: improbable and likely impossible.

Less obvious errors are those caused by careless probe installation. Distances x , x' are usually 1.0 and 0.5 cm, respectively. Small errors in the placement of either of these produces large errors in indicated heat pulse velocity. For example, if x were 0.9 and x' 0.6 cm, Eq. (3) becomes $480/t_0$ rather than $900/t_0$. A ten and 20 percent error in spacing result in a 47 percent error in heat pulse velocity. The best technique, even with careful probe placement, is to measure x , x' in the tree and prepare a separate equation (3) for each measurement locus.

Heat loss from the measurement section is an important but not obvious source of error. Fortunately, the effect of heat loss is more noticeable at low heat pulse velocities, than at high ones. Therefore the absolute error is small. A series of tests to determine how long it takes for a 10-W second heat pulse to dissipate to undetectability showed that the minimum time

was 300s, the maximum well over 1800. My field practice has been to stop all readings at 300 s. The lowest acceptable HPV with a probe spacing of $x = 1.00$ cm, $x' = 0.50$ cm, is

$$\text{HPV} = 900/300 = 3.0 \text{ cm/h} \quad (11)$$

Experience in using the instrumentation with a particular set of probes will allow longer t_0 's.

CONCLUSIONS

A thermal flowmeter for measuring heat pulse velocity consists of a heat source, temperature sensing probes, an indicator of temperature difference and a second timer. Practical field instrumentation can be built with readily available electronic parts.

Heat pulse velocity through a tree stem is indicative of evaporation rates at the leaf surfaces of trees. The magnitude of indicated measurements is less than the magnitude of the actual flow. Indicated magnitude is influenced by the size of probes placed in the stem. Larger probes apparently indicate less flow than smaller ones. There appears to be a consistent and predictable relationship between probe size and error percent but more absolute flow measurements are needed to confirm and define the relationship.

Acknowledgment

The author acknowledges with thanks the use of data obtained while he was a staff member of the Rocky Mountain Forest and Range Experiment Station, U.S. Forest Service, Fort Collins, Colorado.

References

- ¹D. C. Marshall, *Plant Physiology* 33, 385 (1958).
- ²R.H. Swanson, *Flow, Its Measurement and Control in Science and Industry* 1, 1425 (1974).